



TIDE Mass_0

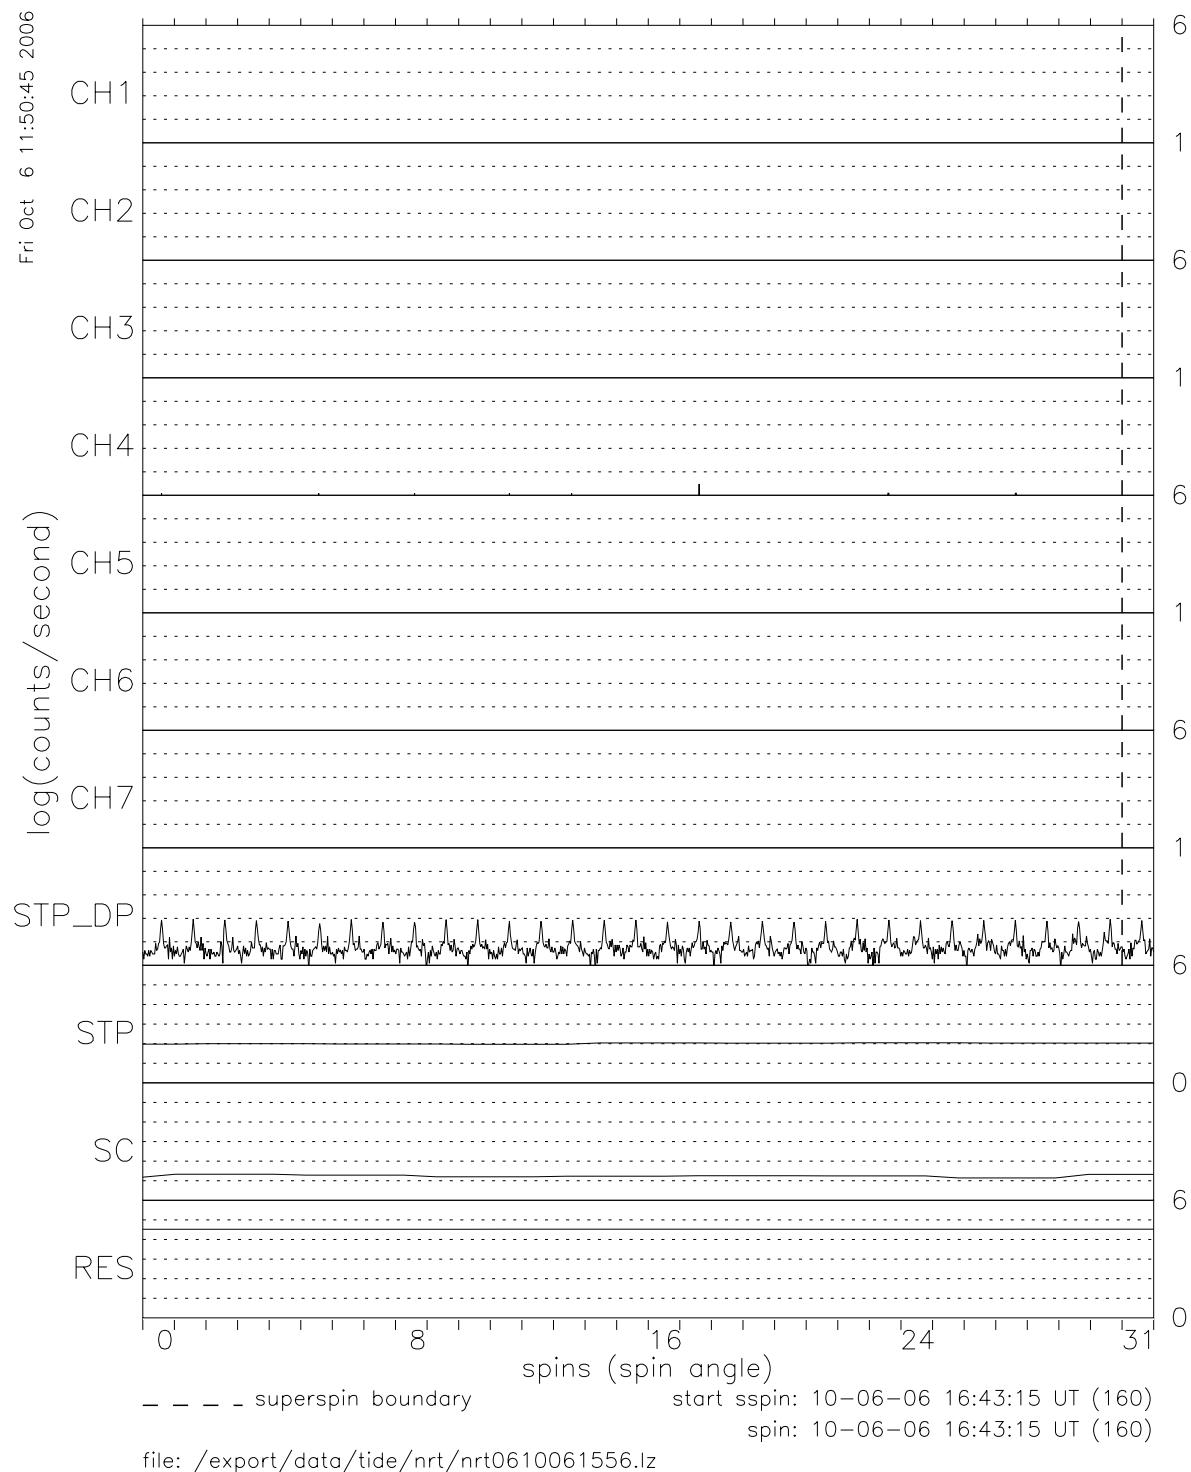

-15kV TOF: -9245 v
 -3.6kV MCP: -3364 v
 -2.4kV MCP: -1784 v
 Input Cur: 306 ma
 RPA max: 237 v
 Mirror max: 238 v

Fri Oct 6 11:50:45 2006

TIDE Direct Events

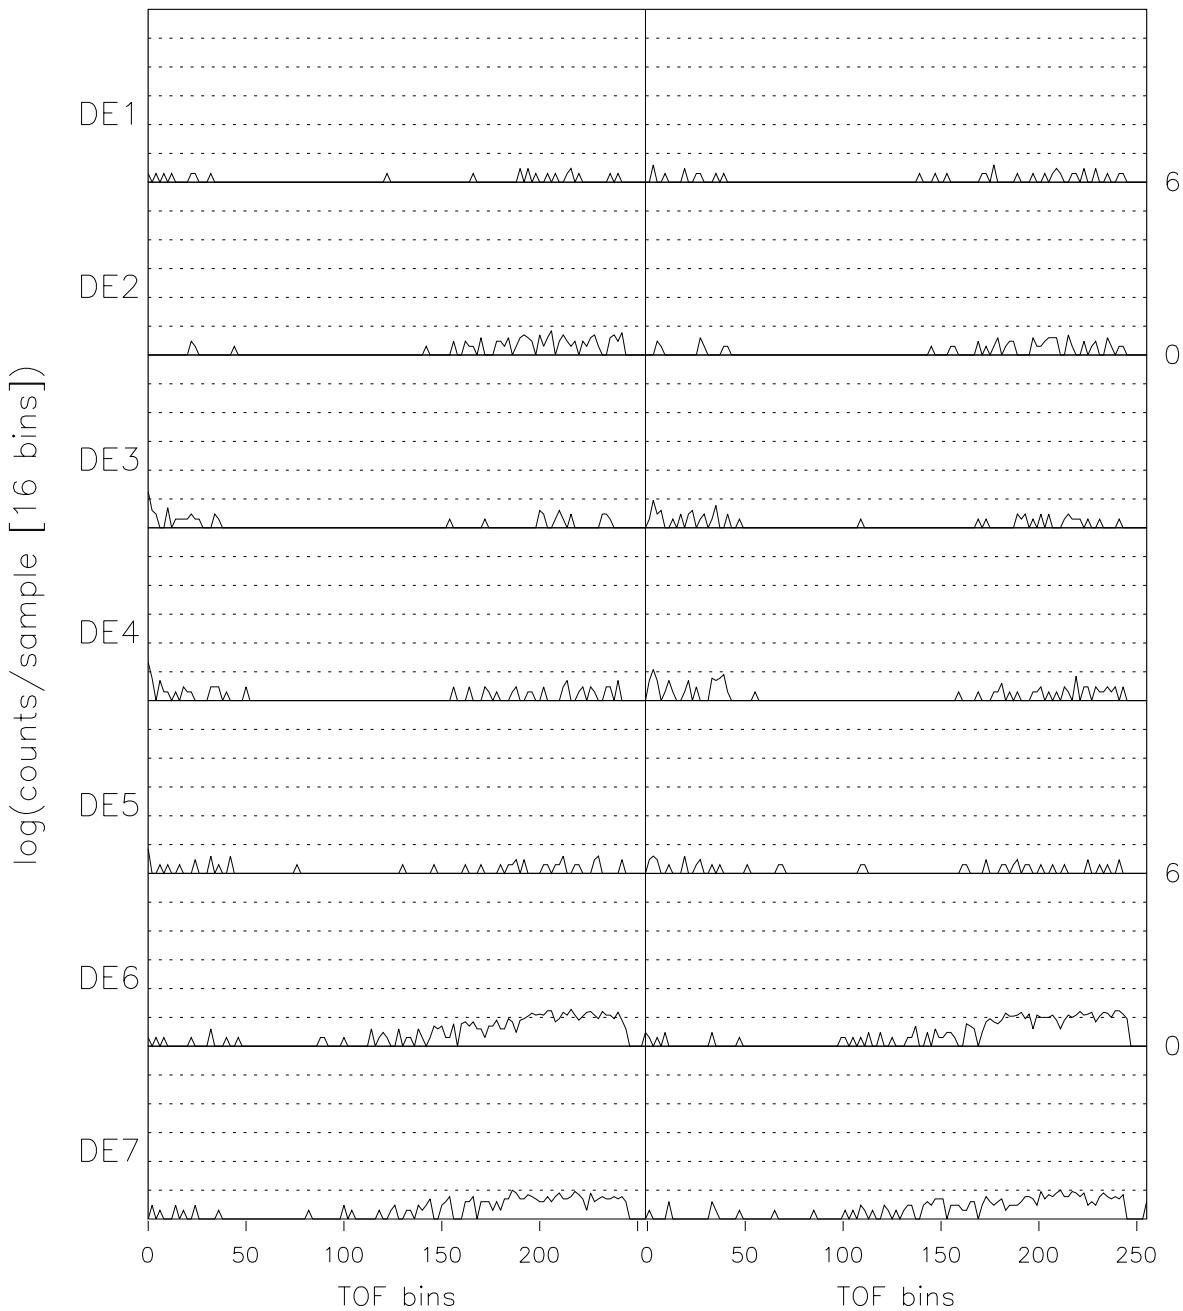

reported: 10-06-06 16:36:44 UT

reported: 10-06-06 16:39:57 UT

file: /export/data/tide/nrt/nrt0610061556.lz

-15kV TOF: -9181 v
-3.6kV MCP: -3379 v
-2.4kV MCP: -1784 v
Input Cur: 296 ma
RPA max: 237 v
Mirror max: 238 v